




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : G01N 27/416	A1	(11) International Publication Number: WO 00/67011 (43) International Publication Date: 9 November 2000 (09.11.00)
(21) International Application Number: PCT/SG99/00038 (22) International Filing Date: 30 April 1999 (30.04.99) (71) Applicant (for all designated States except US): HW ELECTROCHEM TECHNOLOGY PTE LTD. [SG/SG]; 21 Science Park Road #03-17, The Aquarius, Singapore Science Park II, Singapore 117628 (SG). (72) Inventor; and (75) Inventor/Applicant (for US only): GE, Hailin [CN/SG]; Block 284, 3 Choa Chu Kang Avenue #09-336, Singapore 680284 (SG). (74) Agent: MCCALLUM, Graeme, David; Lloyd Wise, Tanjong Pagar, P.O. Box 636, Singapore 910816 (SG).		(81) Designated States: CN, SG, US, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). Published <i>With international search report.</i>

(54) Title: APPARATUS FOR VOLTAMMETRIC ANALYSIS

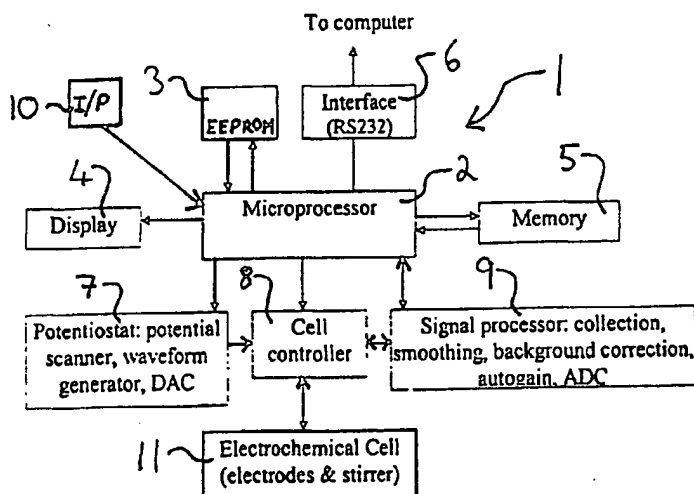

(57) Abstract

Apparatus (1) for voltammetric analysis includes a processor (2) and a first memory device (3) coupled to the processor (2). The first memory device (3) comprises a programmable read only memory and stores a number of electrochemical cell control programs. An output device (4), an input device (10), a second memory device (5) and an electrochemical cell controller (7, 8, 9) are also coupled to the processor (2). The cell controller (7, 8, 9) is adapted to be coupled to an electrochemical cell (11). The processor (2), in response to an analyte input signal entered via the input device (10), retrieves a corresponding electrochemical cell control program, and instructs the cell controller (7, 8, 9) to apply a scanning voltage to the electrochemical cell (11), in accordance with the retrieved control program. The processor (2) also processes output signals received by the cell controller (7, 8, 9) from the electrochemical cell (11), in response to the applied scanning voltage, to obtain an indication of the concentration of an analyte, corresponding to the analyte input signal, in the electrochemical cell (11), and outputs the indication to the output device (4).

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

APPARATUS FOR VOLTAMMETRIC ANALYSIS

The invention relates to apparatus for voltammetric analysis.

Voltammetric analysis is a widely used electroanalytical technique. The art of this technique has been well described in many publications [1,2]. Voltammetric analysis can be carried out using various waveforms, for example, linear, pulse, square and AC or using various operation modes, for example cyclic voltammetry and stripping voltammetry [3]. Many inventors have disclosed specific devices and methods for voltammetric analysis. Girault [4] showed a device for change of electrodes. Fidler et al [5] disclosed a circuit to maintain a stable potential difference between the working and the reference electrodes. Tur Yan et al [6] used a special cell to detect trace metals using stripping voltammetry. Saloheimo et al [7] introduced ultrasonic vibration during pre-electrolysis in stripping voltammetry. Other researchers have designed special electrodes for anodic stripping voltammetry [8-10].

Kissinger [11] predicted the future of electroanalytical instrumentation as being computerization, miniaturization and automation. Computers have been used to collect electrochemical signals [12], to acquire data and control experiments [13] and to modify waveforms [14]. Computerised voltammetric instruments are now commercially available from many instrument manufacturers.

However, computerised voltammetric instruments are generally large in size and costly. Small polarographic or voltammetric analysers are available for specific analytes, such as aldehyde [15] and lead [16]. Multi-element analysis using this type of equipment can be achieved by using multichannel selection [17] or multi-electrodes [18]. However, the number of elements that can be analysed is physically limited.

In addition, the process of voltammetric analysis often involves many decision making steps. Although computerised voltammeters can run analysis automatically it is still necessary for the supporting electrolytes, calibration standards and experimental conditions, such as initial potential, final potential, scan rate and current range, to be chosen by an operator before the analysis commences. During analysis, voltammograms with peak currents or peak areas need to be acquired, and after analysis, the data requires processing and the results reported. These decision making steps require trained personnel with knowledge and experience. Although they can be simplified into a computer program as demonstrated by De kreuk et al [19] in an automatic stripping voltammetric method, as indicated by some researchers [20], automation of voltammetric instrument is a more complicated task than that of other electroanalytical techniques. Hence, automation is often at the level of operation rather than the decision making process.

Therefore, even computerised and highly automated systems

still require skilled and experienced personnel to operate them.

In addition, conventional electrodes for voltammetry have the problem that it is difficult to ensure good electrical contact between the electrode and the electrical wire coupling the electrode to the analysing equipment. In particular, with some types of electrode, such as glassy carbon, it is not possible to solder the electrical wire to the electrode. Accordingly, conventional methods of electrically contacting the wire to the electrode include using mercury to bond the wire to the electrode or using conductive glue. Mercury has the disadvantage that it is toxic and the conductive glue has the disadvantage that it is not easy to disconnect the conductor from the electrodes.

In accordance with a first aspect of the present invention, apparatus for voltammetric analysis comprises a processor; a first memory device coupled to the processor, the first memory device comprising a programmable read only memory and storing a number of electrochemical cell control programs; an output device coupled to the processor; an input device coupled to the processor; a second memory device coupled to the processor; an electrochemical cell controller coupled to the processor, the cell controller being adapted to be coupled to an electrochemical cell; the processing device, in response to an analyte input signal entered via the input device, retrieving a corresponding electrochemical cell control

program, and instructing the cell controller to apply a scanning voltage to an electrochemical cell coupled to the cell controller in use, in accordance with the retrieved control program, and processing output signals received by the cell controller from the electrochemical cell, in response to the applied scanning voltage, to obtain an indication of the concentration of an analyte, corresponding to the analyte input signal, in the electrochemical cell, and outputting the indication to the output device.

Preferably, the programmable read only memory is an electrically erasable programmable read only memory (EEPROM).

Preferably, the output device comprises a display device, such as a liquid crystal display (LCD). However, alternatively or in addition, the output device may comprise an interface device which permits the processor to communicate with another processing device, such as a computer, or with a storage device, such as a magnetic disk or tape drive.

Preferably, the cell controller includes a potentiostat and a signal processor.

Preferably, the apparatus is for stripping voltammetric analysis of an analyte in an electrochemical cell.

In accordance with a second aspect of the present invention, an electrochemical cell comprises a container comprising a

bottom portion, an upper portion and an opening to permit a liquid to be analysed to be introduced into the container; a stirring device depending from the upper portion into the bottom portion of the container; and a counter electrode and a working electrode depending from the upper portion into the bottom portion of the container.

Preferably, the axis of rotation of the stirring device is substantially co-axial with the central vertical axis of the container and the counter and working electrodes are arranged around the stirring device.

Typically, the upper portion of the container, may be separated from the bottom portion of the container to permit liquid to be inserted into the container prior to engagement of the upper portion with the bottom portion.

Typically, the bottom portion may be in the form of a jar or other liquid containing device and the upper portion may form a lid for the jar or containing device.

Preferably, the electrochemical cell further comprises a reference electrode which also depends from the upper portion of the container such that the reference electrode is adjacent the stirring device and located between the counter and the working electrodes.

Preferably, the electrochemical cell is adapted to be used

with the apparatus in accordance with the first aspect of the invention.

In accordance with a third aspect of the present invention, a coupling device for electrically coupling a conductor to an electrode for an electric chemical cell comprises a first conducting member; a second conducting member, electrically coupled and movably coupled to the first conducting member; and a biasing device to bias the first and the second member away from each other; the first conducting member being adapted to be coupled to an electrical conductor and the second member having an engagement portion adapted to engage with and electrically couple the second member an electrode for an electrochemical cell.

Preferably, one of the first and the second members is slidably located within the other of the first and the second members such that the engagement portion of the second portion is biased away from the first member by the biasing device. Typically, the second member is slidably located within the first member.

Preferably, the engagement surface of the second member is of a material which provides a low electrical contact resistance with the material of the electrode with which the engagement surface is to be engaged. For example, the material of the engagement portion may be a material which is harder than the material of the electrode, such as titanium or iridium, or a

material which has a low susceptibility to oxidation, such as gold.

Typically, the first member may include an aperture in the first member adapted to receive a generally cylindrical electrically conducting member such that the conducting member when inserted into the aperture is electrically coupled to the first member.

An example of apparatus for voltammetric analysis in accordance with the invention will now be described with reference to the accompanying drawings, in which:-

Figure 1 is a schematic diagram of apparatus for voltammetric analysis;

Figure 2 is a side view of an electrochemical cell for use in the apparatus of Figure 1;

Figure 3 is a cross-sectional view of an upper portion of the electrochemical cell shown in Figure 2;

Figure 4 is a front view of the upper portion shown in Figure 3;

Figure 5 is a cross-sectional view of an electrode for use in the cell shown in Figures 2 to 4;

Figure 6 shows the apparatus of Figure 1 incorporated into a handheld voltammetric analyser;

Figure 7 shows the apparatus of Figure 1 incorporated into an on-line voltammetric analyser;

Figure 8 is a flow diagram illustrating the operation of

a diagnostic program for use with the apparatus shown in Figures 1, 6 and 7; and,

Figure 9 is a graph showing calibration results and test results obtained using the analyser shown in Figure 6.

Figure 1 is a block diagram of voltammetric analysis apparatus 1 which includes a microprocessor 2, an electrically erasable programmable read only memory (EEPROM) 3, a display device 4 such as a liquid crystal display device, a memory device 5 which may be a random access memory (RAM), an interface device 6 such as an RS 232, a potentiostat 7, a cell controller 8, a signal processor 9, and an input device, such as a keypad 10.

The cell controller 8 is adapted to be coupled to an electrochemical cell 11 which is generally in the form of a container with electrodes 14, 15, 16 and a stirrer 17. An example of an electrochemical cell 11 suitable for use with the apparatus shown in Figure 1 is shown in more detail in Figures 2 to 4.

The interface device 6 permits the apparatus 1 to be linked to a computer, for example, to permit programming of the EEPROM 3 or to permit downloading of the memory 5 to a more permanent storage device in the form of for example, magnetic media such as a magnetic disk or tape.

The potentiostat 7 is coupled to the microprocessor 2 and generates a scanning potential which is modified with various

waveforms such as DC, AC, square wave or differential pulse, in accordance with a chosen program downloaded from the EEPROM 3 to the microprocessor 2.

The cell controller 8 is coupled to the microprocessor 2 and contains a group of switches. According to the chosen program it will switch on or off the electrochemical cell 11 to allow potential generated by the potentiostat 7 to be applied to the electrodes 14, 15, 16 and to allow signals detected by the electrodes 14, 15, 16 to be received by the signal processor 9. It also turns on and off the stirrer 17.

The signal processor 9 is coupled to the microprocessor 2. In accordance with the chosen program it will receive signals from the cell 11, process the signals, convert them into digital information, and pass them to the microprocessor 2 to be stored by the microprocessor 2 in the memory 5.

As shown in Figure 2, the electrochemical cell 11 includes a container comprising a vessel 12 and an electrode holder 13 in the form of a lid for the vessel 12. The lid 13 supports a working electrode 14, a reference electrode 15 and a counter electrode 16 as well as the stirring device 17. The stirring device 17 comprises an electric motor 18 mounted on top of the lid 13, a drive shaft 19 extending through the lid 13 into the vessel 12 and a rotor 20 located at the end of the drive shaft 19 and adjacent to lower ends of the electrodes 14, 15, 16.

Typically, the stirrer 17 is a 0.1W stirrer and the vessel 12 is a glass bottle with a volume of approximately 20ml. The working electrode 14 may be a 3mm diameter disc glassy carbon electrode, the counter electrode 16 may be a 3mm x 3mm platinum electrode and the reference electrode 15 may be a Ag/AgCl electrode.

The reference electrode 15 has a conventional reference electrode construction. A cross-sectional view of the electrode construction for the working and counter electrodes 14, 16 is shown in Figure 5. As shown in Figure 5, each of the electrodes 14, 16 comprise an electrode sensing material 50 held in an electrode body 51. In the electrodes 14, 16 the sensing material 50 is glassy carbon and platinum, respectively. The body 51 encloses a coupling device which comprises an outer casing 52, a contact pin 53 slidably mounted within the casing 52 and a biasing device 54 within the casing 52. The biasing device 54 acts to bias the pin 53 to an extended position in which a contact point 55 of the pin 53 is biased against the sensing material 50 to make electrical contact with the sensing material 50. The pin 53, biasing device 54 and casing 52 are all electrically conducting and the end of the casing 52, opposite to the end from which the pin 53 extends, is electrically coupled to a wire 56 which couples the sensing material 50 to the controller 8.

In order to ensure a good electrical contact between the

contact point 55 and the sensing material 50, the pin 53, or at least the contact point 55, is formed from a material which is harder than the sensing material 50. This helps ensure a good electrical contact as the contact point 55 "bites" into the sensing material 50. For example, the pin 53 could be manufactured from titanium or iridium.

The lid 13 of the cell 11 is shown in more detail in Figure 3 which shows a cross-sectional view of the lid 13 and Figure 4 which shows a top view of the lid 13. The lid includes a central through bore 21 through which the drive shaft 19 extends and four side through bores 22, 23, 24, 25. The working electrode 14 extends through the bore 23, the reference electrode 15 extends through the bore 24 and the counter electrode 16 extends through the bore 25. The bore 22 is left empty and may be used for introduction of analyte and/or electrolyte into the vessel 12.

Due to the relative simplicity of the apparatus 1, the apparatus can be incorporated into a relatively small handheld analyser 30 as shown in Figure 6. The typical dimensions of the handheld analyser 30 are 40mm x 100mm x 200mm and the overall weight is typically approximately 0.5kg.

The handheld voltammetric analyser 30 incorporates the apparatus shown in Figure 1 with the exception of the electrochemical cell 11. In particular, the handheld voltammetric analyser 30 includes the LCD display 4, the

keypad 10, the communication interface 6 and a port 31 which permits the analyser 30 be connected to an external power supply.

However, as an alternative to, or in addition to, the external power supply, the handheld analyser 30 may be powered by an internal battery, such as any form of suitable conventional rechargeable battery. Typically, the battery may be recharged by the external power supply via the port 31 when necessary.

The remainder of the components, including the microprocessor 2, the EEPROM 3, the RAM 5, the potentiostat 7, the cell controller 8 and the signal processor 9 are contained within the housing of the analyser 30.

The handheld analyser 30 also has a communication port 33 which is coupled to the electrochemical cell 11 in use and is coupled internally to the cell controller 8. This permits the cell controller 8 to control the scanning voltage applied to the electrochemical cell and to receive the output signals from the electrochemical cell in response to the applied scanning voltage. In addition, the handheld analyser 30 may optionally be connected through the interface 6 to a remote computer, for example, to transfer data to the remote computer and/or to be remotely controlled by the remote computer.

In addition, the apparatus shown in Figure 1 can be incorporated into an on-line voltammetric analyser 60 as shown

in Figure 7. The on-line analyser 60 is coupled via the interface 6, local controller 34 and interface 35, to a remote computer 36 which is used to remotely control the analyser 60. The analyser 60 and the local controller 34 are powered by a power supply 32 which may be battery operated or powered by a mains power supply 37. In the analyser 60, the key board 10 is omitted, as instructions may be entered into the analyser 60 via the remote computer 36. However, apart from the omission of the key board 10, the analyser 60 is identical to the handheld analyser 30, described above and shown in Figure 6. The on-line analyser 60 is coupled via cable 61 and connection port 33 to the electrochemical cell 11 and to metering pumps 62, 63, 64, 65, 66 which can be operated to pump liquid from reagent reservoirs 67, 68, 69, a sampling valve 70 and a rinsing water valve 71, respectively into the electrochemical cell 11. In addition, a vent valve 72 in the electrochemical cell 11 can also be controlled by the remote computer 36 or by local controller 34.

The liquid containing the sample to be analysed is connected to the sampling valve 70, clean water is connected to the rinsing valve 71 and standard reagents are stored in the reagent reservoirs 67, 68, 69. The vent valve 72 is used to empty the electrochemical cell 11 of liquid.

In use, the handheld analyser 30 and the on-line analyser 60 are set up by programming into the EEPROM 3 digital information corresponding to the configuration of the

electrochemical cell 11 to be used with the analyser 30, 60. Such information includes details of the working electrode, reference electrode, stirrer and vessel. For example, typical information may be that the cell contains a 3mm diameter disc glassy carbon electrode, a 3mm by 3mm platinum counter electrode, a Ag/AgCl reference electrode, a 0.1W stirrer, a 20ml vessel and an electrode holder to fix each electrode position.

The second step is to formulate a reagent with a known composition as a testing media and convert it into digital information. The formulated reagent will contain a standard analyte, a buffer, a masking agent, a supporting electrolyte, a preservative and a performance enhancer. The standard analyte with known concentration is used to calibrate the cell 11. The concentration range is typically from 1ppb to 1000ppm. The buffer is used to control pH and usually contains a salt and an acid or a base. The masking agent is used to reduce interference from samples, which may be a complex agent, an organic solvent, a precipitation agent, a redox agent, a salt, etc. The supporting electrolyte is an ionic compound to provide conductivity. The preservative prolongs shelf life of the reagent. The performance enhancer can increase selectivity and sensitivity of the reagent.

A voltammetric analysis is then performed under fixed experimental conditions such as scan waveform, initial potential, scan rate, final potential, current range, etc.

This arrangement makes a voltammetric response position (potential) easily identifiable. The conditions can be obtained according to published papers, previous experience and expert knowledge. All data is converted into digital information.

Voltammetric response is searched for automatically by the analyser 30, 60. The voltammetric response potential is determined for the highest current reading in a certain time period while voltammetric response current is calculated by subtracting background current from current reading. This procedure is programmed into the EEPROM 3.

System testing is then performed using the standard reagent. As cell configuration, testing media and experimental conditions are fixed, voltammetric response to the analyte in the testing media should be a constant. Any significant changes of response potential or current will indicate system errors such as reference electrode failure or working electrode fouling. The purpose of the system testing step is to find and display these errors by comparing measured values with pre-set values. This procedure is programmed into the EEPROM 3.

The electrodes are then calibrated automatically. Voltammetric analysis of the standard reagent is carried out in the testing media. The response potential and current is stored. This procedure makes sure that the electrodes are

calibrated just before sample analysis so that the electrode surface condition remains unchanged. This calibration procedure is programmed into the EEPROM 3.

A test sample is then analysed. This is performed by voltammetric analysis of a test sample by mixing a known volume of the test sample with a known volume of the standard reagent. The response potential and current is compared with stored response for the standard reagent and the result is calculated and reported. This procedure is also programmed into the EEPROM 3.

The EEPROM 3 also includes a diagnostic program which is illustrated schematically in the flow diagram shown in Figure 8. In particular, the diagnostic program checks 70 the results of the analysis to ensure that a peak current is detected in the voltammetric analysis. If the peak current is not detected, the microprocessor displays 71 an error message in the LCD 4 and stops 72 the analysis. The diagnostic program also uses the reference potential value range stored in the data in the EEPROM 3 and compares this with the peak current response at maximum intensity to check 73 the reference electrode status. If the reference potential value is out of range, the analyser outputs 74 an error message to the operator and stops 75 the analysis. The diagnostic program also uses the reference current data in the EEPROM 3 and compares this with the maximum response intensity obtained during analysis to check 76 gain and working electrode status.

If the maximum response intensity detected is out of range of the reference current data, the diagnostic program causes the microprocessor to instruct the signal processor 9 to change 77 to a more suitable gain level and the analysis is continued. If the diagnostic program detects that no gain is available, the microprocessor outputs 78 an error message to the operator and stops the analysis 79. This permits the diagnostic program to optimise the signal collection potential range and current range which is stored in the memory 5.

In addition, the diagnostic program uses the reference data stored in the EEPROM 3 which is compared with the actual peak current response obtained from the standard reagent to determine whether the peak current obtained from standard reagent corresponds to the peak current expected from the standard reagent. In the event that the peak current obtained is outside a certain deviation from the expected peak current, the microprocessor will output an error or warning message to the operator.

After programming of the EEPROM 3, the analyser 30, 60 can be used in conjunction with the cell 11 to run a voltammetric analysis on a particular analyte. Initially, an operator turns on the analyser 30, 60 being used and enters the analyte to be analysed and the concentration of interest. The operator then formulates a standard reagent for the analyte of interest and adds this to the electrochemical cell 11 through the aperture 22.

The analyser 30, 60 then conducts a test on the reagent to check the conditions of the system automatically.

After this test, electrode status and instrument readiness will be reported and some analysis conditions such as gain and peak position will be set automatically. Any system errors detected by the diagnostic program will stop analysis with correction instructions. This enhances the performance and reliability of the apparatus.

As soon as the instrument is ready, the system is calibrated automatically. During the calibration process, the system collects and processes raw data and stores a response which represents a known concentration of the analyte to be tested for in the memory.

After the calibration process, a fixed volume of the test sample is added into the cell 11 and mixed with a fixed volume of the standard reagent. The system then collects and processes the voltammetric raw data again. The response which represents the concentration of the standard plus the sample is stored in the memory. The microprocessor 2 performs a calculation to determine the concentration of the analyte in the test sample using the information from the calibration sample and the result will be reported and displayed.

An example of use of the analyser 30 and cell 11 to analyse the concentration of Cu^{2+} in a waste water sample will now be

described. However, the analyser 60 could be used in the same manner to perform the analysis.

A standard reagent containing 2 ppm copper nitrate, 0.5 M acetic acid, 0.5 M sodium acetate and 20 ppm mercury chloride was prepared. The formulation of the reagent was digitally coded and entered into the EEPROM 3. In addition, a linear anodic stripping voltammetry scan was also programmed into the EEPROM 3 with the following conditions:

- (i) An initial potential of -0.8V;
- (ii) Pre-electrolysis for 30s;
- (iii) A scan rate of 100mVs^{-1} ;
- (iv) A final potential of +0.5V; and
- (v) An electrode cleaning time of 20s at +0.5V.

10ml of the reagent was then introduced into the vessel 12 through the aperture 22 as a standard and the voltammetric analysis process was started using the keypad 10. When started the microprocessor 2 prompts a user via the display 4 to enter the analyte to be tested for. The operator in response to this enters "copper". The microprocessor 2 then prompts a user via display 4 for the concentration of interest and the user enters "1ppm" using the keypad 10. In response to this information, the microprocessor 2 selects the appropriate program stored in the EEPROM 3 for an analyte of copper with a concentration of interest of 1ppm and this is downloaded from the EEPROM into the microprocessor 2. The microprocessor 2 then runs the chosen program and in response

to the program the microprocessor 2 generates control signals to control the output from the potentiostat 7 to the cell controller 8 and the signal processor 9 and the cell controller 8 directly. By causing the cell controller 8 to apply the pre-programmed linear anodic stripping voltammetric conditions (i) to (v) listed above which form part of the program downloaded from the EEPROM 3 into the microprocessor 2. Using the output signals from the reference and counter electrodes 15, 16 which are temporarily stored by the microprocessor 2 in the RAM 5, the microprocessor 2 then analyses the test results and stores the results as a calibration.

After the calibration is completed, the microprocessor 2 prompts a user via the display 4 to add the actual test sample. At this point, the user replaces the 10ml of the standard calibration reagent with 5ml of the calibration reagent and 5ml of the waste water sample to be analysed. The operator then informs the analyser 30 using the keypad 10 that the cell 11 contains the sample to be tested and the analyser repeats the linear anodic stripping voltammetry scan under the same conditions as that conducted for the standard calibration sample.

The microprocessor 2 then compares the results of the test sample with the calibration sample and outputs the concentration of Cu^{2+} found in the test sample by means of the display 4.

In addition, an operator can subsequently or simultaneously download the results to the computer 36 for permanent storage and/or for graphical display and/or printing of the results.

A typical graphical display obtained from the analyser 30 is shown in Figure 9 for the above example. The graph shows the applied voltage versus the sensed current for the calibration sample (A) containing 1ppm Cu^{2+} ions and the waste water sample (B). It can be seen from the graph that sample B has a peak which is approximately 1.5 times greater than the calibration sample A indicating that the concentration of Cu^{2+} ions in the waste water sample B is approximately 2.2ppm. It should be noted that the same graphical display would be obtained using the analyser 60 for the analysis instead of the analyser 30.

In addition to copper, the apparatus 1 and electrochemical cell 11 can be used to detect concentrations of most ions. Examples of typical ions that can be detected are ions of titanium, vanadium, chromium, manganese, iron, cobalt, nickel, zinc, gallium, germanium, arsenic, silver, cadmium, indium, tin, antimony, tungsten, platinum, gold, mercury, thallium, lead and bismuth, as well as organic compounds such as aromatics, aldehydes, alcohols, ketones, ethers, quinones, halides, heterocyclics, nitrocompounds, amines, phenols, organic acids and organic metallics.

In fact the apparatus 1 and the cell 11 can be used to detect any ion which can be detected using conventional voltammetry.

Concentrations that can be detected can be any concentration which can be detected using conventional voltammetric analysis, and typically any concentration in the range from approximately 1ppb to 1000ppm.

References

1. Peter T. Kissinger, William R. Heineman, "Laboratory Techniques in Electroanalytical Chemistry", by Marcel Dekker Inc USA 1996.
2. E.A.M.F Dahmen, "Electroanalysis", Elsevier Science Publishing Co. Inc. USA 1986.
3. Kh. Brainina, E. Neyman, "Electroanalytical Stripping Methods" by John Wley & Sons, Inc. USA 1993
4. US Patent No. 5,686,829, Voltammetric Method and Apparatus.
5. US Patent No. 5,198,771, Potentiostatic Apparatus & Methods.
6. US Patent No. 5,635,043, Device Comprising Microcell for Batch Injection.
7. US Patent No. 4,786,373, Voltammetric Method of Measuring.
8. US Patent No. 4,201,646, Apparatus for Stripping Voltammetry.
9. US Patent No. 4,058,446, Anodic Stripping Voltammetry System & Combination Electrode Assembly Therefore.
10. US Patent No. 3,904,487, Anodic Stripping Voltammetry & Apparatus Therefor.
11. Peter T. Kissinger, The Future of Electroanalytical Instrumentation, "Analyst, May 1994 Vol. 119.

12. US Patent No. 5,644,501, Method of Using a Computer to Collect Chemical Signals Directly.
13. Karsten N. Thomsen, Hans J. Skov, Maria E.R. Dam, "A Flexible Instrument for Voltammetry, Amperometry and Stripping Potentiometry", *Analytica Chimica Acta* 293(1994)1-17.
14. B.Y.Liao, M.S.Young, and C.Y.Wang, "PC-Based Instrument of a Modified Differential Normal Pulse Voltammetry with Background Current Correction Technique" *Rev. Sci. Instrum.*, Vol. 65, No. 5, May 1994.
15. US Patent No. 3,922,205, Portable Polarographic Analyser and Quick Polarographic Determinations.
16. US Patent No. 5,437,772, Portable Lead Detector.
17. Gwyn Williams and Claudius D'Silva, "Hand-Held Instrumentation for Environmental Monitoring" *Analyst*, February 1994, Vol. 119.
18. US Patent No. 5,217,112, Voltammetric Analysis Apparatus and Method.
19. M. Valcarcel, M.D. Luque de Castro "Automatic Methods of Analysis", *Elsevier Science Publishers B.V.* 1988.
20. US Patent No. 4,220,515, Apparatus for Automatically Determining the Amount of One or More Substances in a Liquid.

Claims

1. Apparatus for voltammetric analysis comprising a processor; a first memory device coupled to the processor, the first memory device comprising a programmable read only memory and storing a number of electrochemical cell control programs; an output device coupled to the processor; an input device coupled to the processor; a second memory device coupled to the processor; an electrochemical cell controller coupled to the processor, the cell controller being adapted to be coupled to an electrochemical cell; the processor device, in response to an analyte input signal entered via the input device, retrieving a corresponding electrochemical cell control program, and instructing the cell controller to apply a scanning voltage to an electrochemical cell coupled to the cell controller in use, in accordance with the retrieved control program, and processing output signals received by the cell controller from the electrochemical cell, in response to the applied scanning voltage, to obtain an indication of the concentration of an analyte, corresponding to the analyte input signal, in the electrochemical cell, and outputting the indication to the output device.

2. Apparatus according to claim 1, wherein the programmable read only memory is an electrically erasable programmable read only memory.

3. Apparatus according to claim 1 or claim 2, wherein the

output device comprises a display device.

4. Apparatus according to any of the preceding claims, wherein the output device comprises an interface device which permits the processor to communicate with another processing device.

5. Apparatus according to any of the preceding claims, wherein the cell controller further comprises a potentiostat and a signal processor.

6. Apparatus according to any of the preceding claims, wherein the apparatus is for stripping voltammetric analysis.

7. An electrochemical cell comprises a container comprising a bottom portion, an upper portion and an opening to permit a liquid to be analysed to be introduced into the container; a stirring device depending from the upper portion into the bottom portion of the container; and a counter electrode and a working electrode depending from the upper portion into the bottom portion of the container.

8. An electrochemical cell according to claim 7, wherein the axis of rotation of the stirring device is substantially coaxial with the central vertical axis of the container and the counter and working electrodes are arranged around the stirring device.

9. An electrochemical cell according to claim 7 or claim 8, wherein the upper portion of the container is disengageable from the bottom portion of the container.
10. An electrochemical cell according to any of claims 7 to 9, wherein the bottom portion forms a liquid containing device and the upper portion forms a lid for the bottom portion.
11. An electrochemical cell according to any of claims 7 to 10, further comprising a reference electrode depending from the upper portion of the container such that the reference electrode is adjacent the stirring device and located between the counter and the working electrodes.
12. Apparatus according to any of claims 1 to 6, and further comprising an electrochemical cell in accordance with any of claims 7 to 11.
13. A coupling device for electrically coupling a conductor to an electrode for an electric chemical cell comprises a first conducting member; a second conducting member, electrically coupled and movably coupled to the first conducting member; and a biasing device to bias the first and the second member away from each other; the first conducting member being adapted to be coupled to an electrical conductor and the second member having an engagement portion adapted to engage with and electrically couple the second member an electrode for an electrochemical cell.

14. A coupling device according to claim 13, wherein one of the first and the second members is slidably located within the other of the first and the second members such that the engagement portion of the second portion is biased away from the first member by the biasing device.

15. A coupling device according to claim 14, wherein the second member is slidably located within the first member.

16. A coupling device according to any of claims 13 to 15, wherein the engagement surface of the second member is of a harder material than the material of electrode with which the engagement surface is to be engaged.

17. A coupling device according to any of claims 13 to 16, wherein, the first member includes an aperture adapted to receive a generally cylindrical electrically conducting member such that the conducting member when inserted into the aperture is electrically coupled to the first member.

1/6

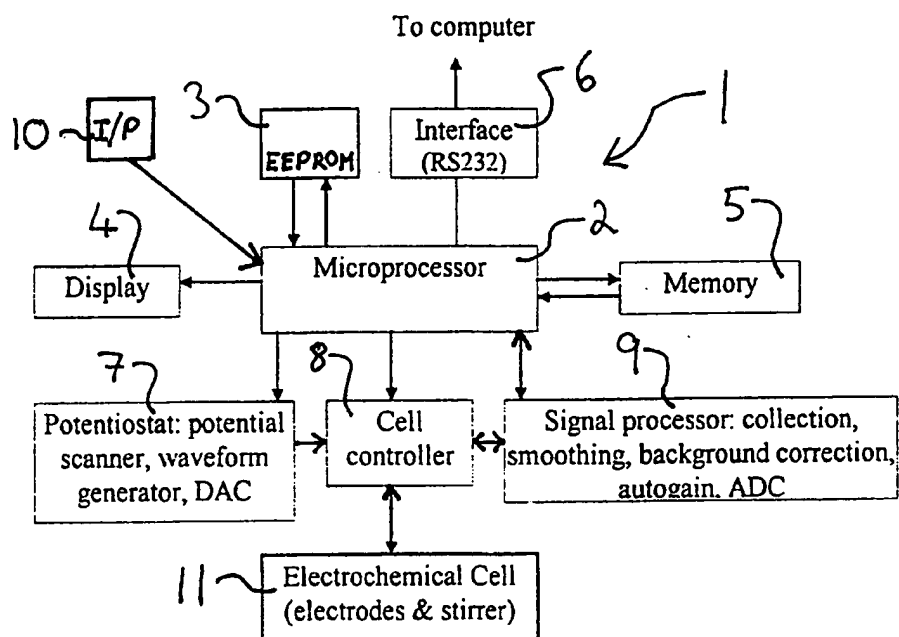


Figure 1

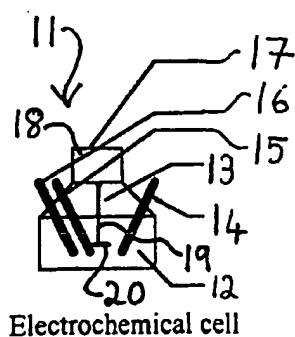


Figure 2

2/6

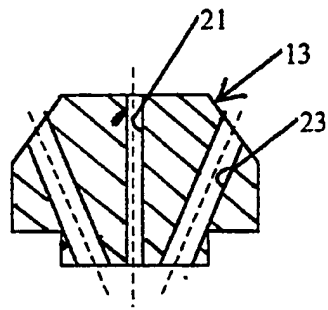


Figure 3

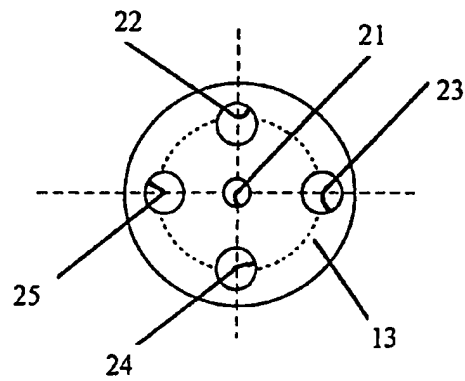


Figure 4

3/6

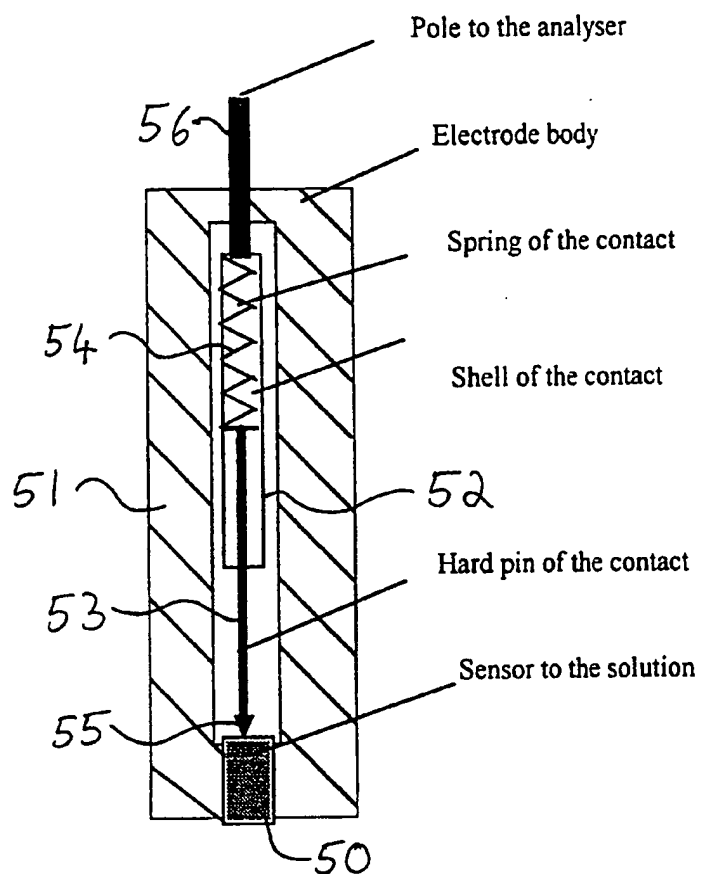


Figure 5

4/6

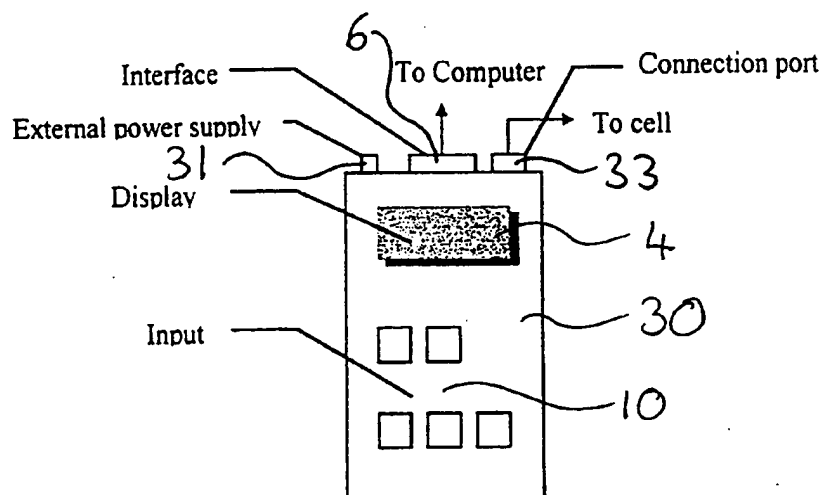


Figure 6

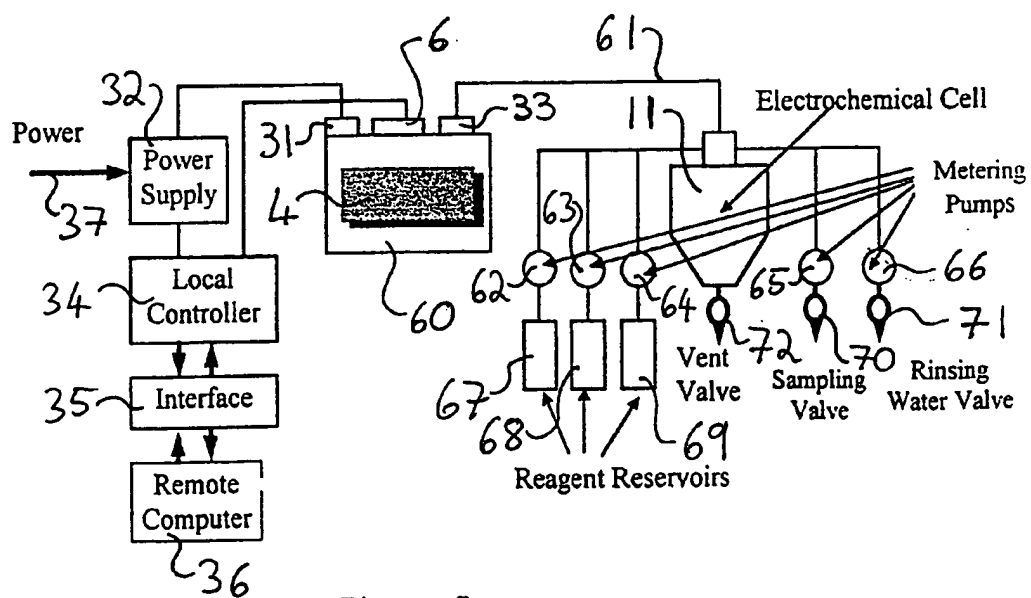


Figure 7

5/6

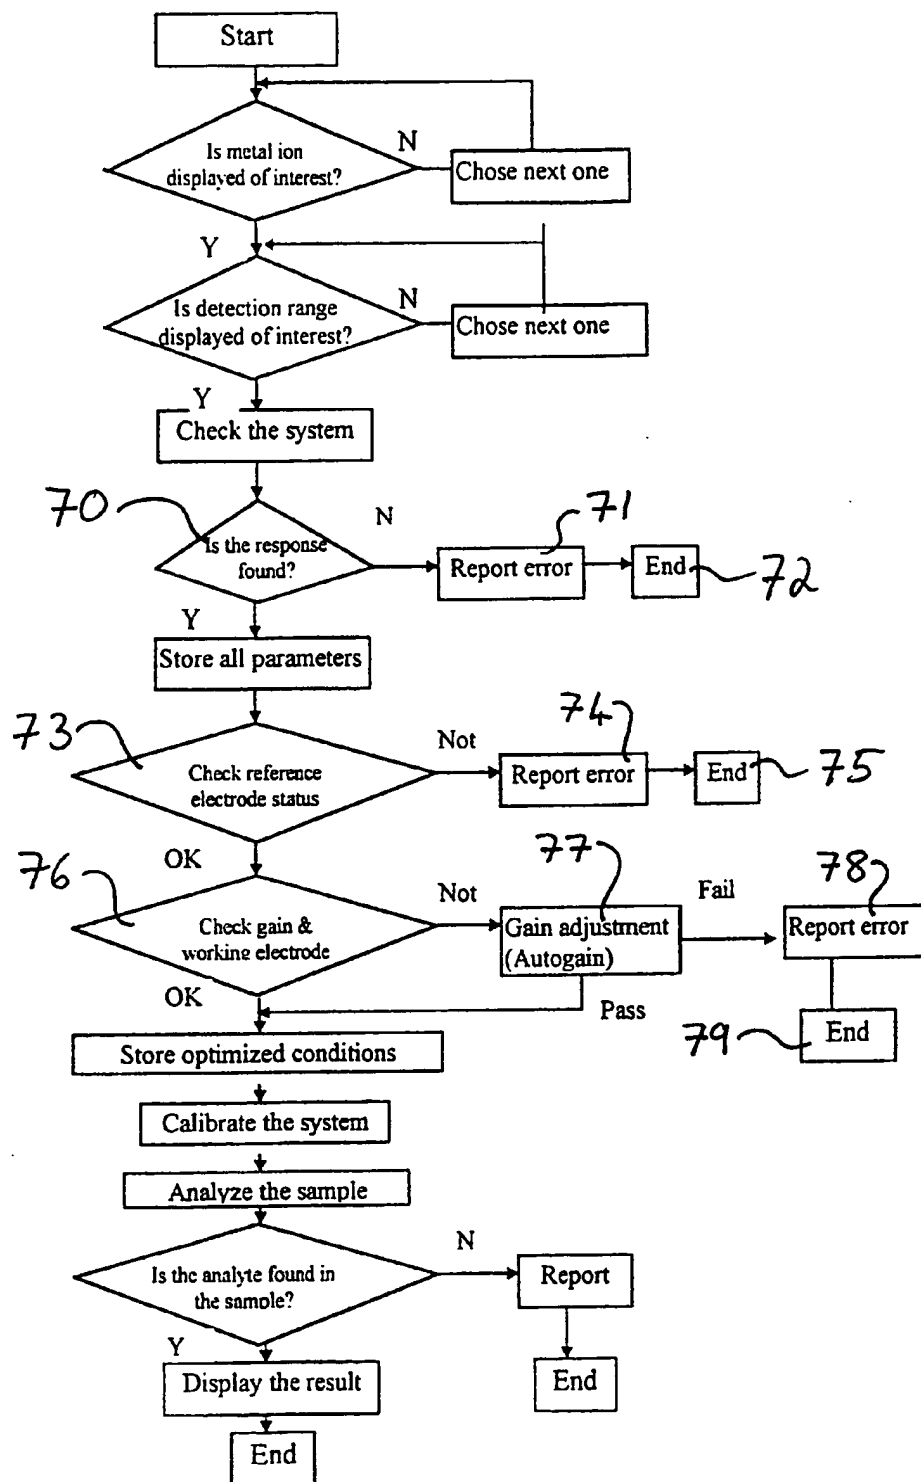


Figure 8

6/6

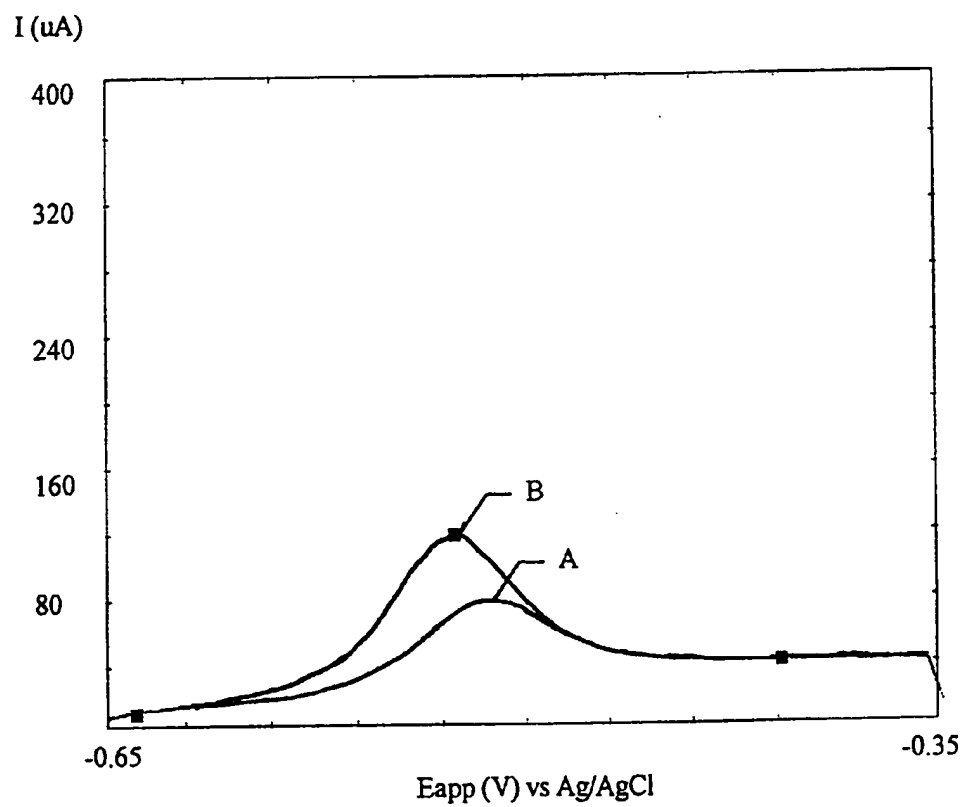


Figure 9

INTERNATIONAL SEARCH REPORT

International application No.
PCT/SG 99/00038

A. CLASSIFICATION OF SUBJECT MATTER		
IPC ⁷ : G 01 N 27/416		
According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED		
Minimum documentation searched (classification system followed by classification symbols)		
IPC ⁷ : G 01 N 27/416		
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched		
Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)		
WPI		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 98/36270 A2 (CHAMPAGNE), 20 August 1998 (20.08.98).	1
A	DE 2336402 A1 (CENTRALEC), 06 February 1975 (06.02.75).	7
A	RU 2069360 C1 (IVA CO LTD.), 20 November 1996 (20.11.96), Russian Patent Abstracts, Section S-X, week 9728, London: Derwent Publications Ltd., Class S03, AN 1997-256172.	13

<input type="checkbox"/> Further documents are listed in the continuation of Box C. <input checked="" type="checkbox"/> See patent family annex.		
* Special categories of cited documents: „A“ document defining the general state of the art which is not considered to be of particular relevance „E“ earlier application or patent but published on or after the international filing date „L“ document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) „O“ document referring to an oral disclosure, use, exhibition or other means „P“ document published prior to the international filing date but later than the priority date claimed „T“ later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention „X“ document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone „Y“ document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art „&“ document member of the same patent family		
Date of the actual completion of the international search		Date of mailing of the international search report
19 January 2000 (19.01.00)		16 February 2000 (16.02.00)
Name and mailing address of the ISA/AT Austrian Patent Office Kohlmarkt 8-10; A-1014 Vienna Facsimile No. 1/53424/200		Authorized officer Nardai Telephone No. 1/53424/347

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/SG 99/00038

Patent document cited in search report			Publication date	Patent family member(s)			Publication date
WO	A2	9836270	20-08-1998	AU	A1	40057/97	08-09-1998
WO	A3	9836270	08-10-1998	US	A	5980708	09-11-1999
DE	A1	2336402	06-02-1975	none			
RU	C1	2069360	20-11-1996	none			